

## (12) INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

(19) World Intellectual Property  
Organization  
International Bureau



(43) International Publication Date  
1 April 2004 (01.04.2004)

PCT

(10) International Publication Number  
**WO 2004/026395 A1**

(51) International Patent Classification<sup>7</sup>: A61N 1/36, 1/08

Hans [SE/SE]; Landsvägen 51, S-17265 Sundbyberg (SE).

(21) International Application Number:

PCT/SE2003/001082

(74) Common Representative: ST JUDE MEDICAL AB;  
Patent Department, Veddestavägen 19, S-17584 Järfälla (SE).

(22) International Filing Date: 23 June 2003 (23.06.2003)

(25) Filing Language:

English

(81) Designated State (*national*): US.

(26) Publication Language:

English

(84) Designated States (*regional*): European patent (AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HU, IE, IT, LU, MC, NL, PT, RO, SE, SI, SK, TR).

(30) Priority Data:

0202803-3 23 September 2002 (23.09.2002) SE

(71) Applicant (*for all designated States except US*): ST JUDE MEDICAL AB [SE/SE]; Veddestavägen 19, S-17584 Järfälla (SE).

Published:


— with international search report

(72) Inventor; and

(75) Inventor/Applicant (*for US only*): STRANDBERG,

*For two-letter codes and other abbreviations, refer to the "Guidance Notes on Codes and Abbreviations" appearing at the beginning of each regular issue of the PCT Gazette.*

(54) Title: IMPLANTABLE MEDICAL DEVICE

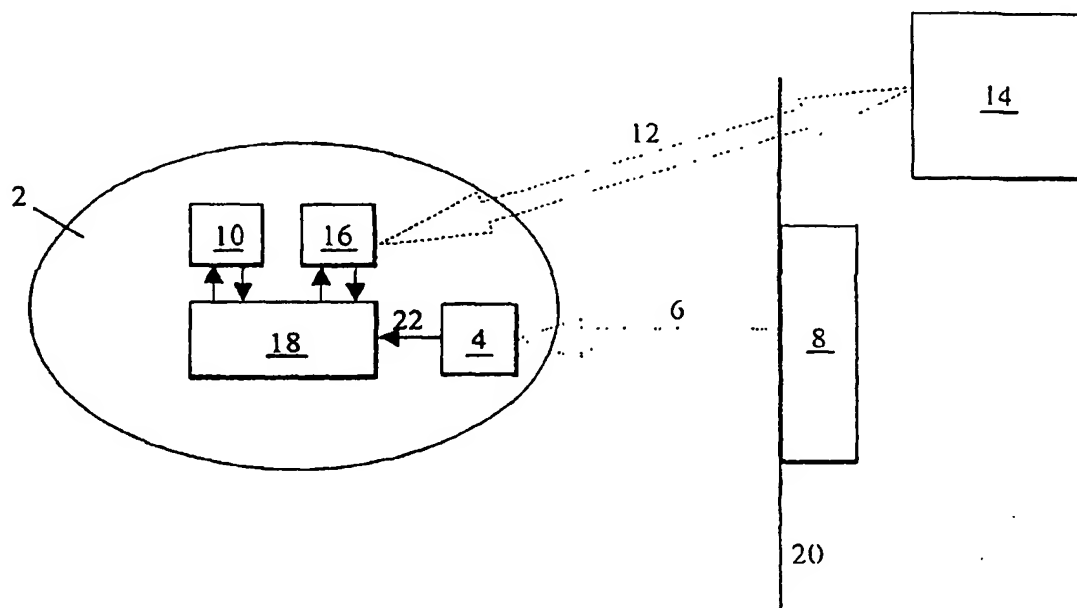

(57) Abstract: Implantable medical device adapted to be operated in a normal mode of operation and in at least one other mode of operation and provided with a signal detecting means responsive of an external activation. The medical device is provided with a special timing means adapted to be programmed with a specified time period, wherein the device is adapted to enter said one other mode of operation being a predefined special mode of operation if an external activation is detected by said signal detecting means during said specified time period, and that the device is adapted to enter a normal test mode of operation if an external activation is detected by said signal detecting means outside said specified time period.